

SCHOTT[®] Instruments
Einstabmesskette

K 60

Kalium Einstabmesskette K 60

Seite 2

Potassium Combination Electrode K 60

Page 12

**Aktualität bei
Drucklegung**

Fortschrittliche Technik und das hohe Qualitätsniveau unserer Produkte werden durch eine ständige Weiterentwicklung gewährleistet. Daraus können sich evtl. Abweichungen zwischen dieser Bedienungsanleitung und Ihrer Einstabmesskette ergeben. Auch Irrtümer können wir nicht ganz ausschließen. Haben Sie deshalb bitte Verständnis, dass aus den Angaben, Abbildungen und Beschreibungen keine juristischen Ansprüche abgeleitet werden können.

Garantieerklärung

Bei ordnungsgemäßer Handhabung übernimmt SI Analytics für die Dauer eines Jahres die Gewährleistung für die Qualität der Elektrode bzw. Messkette.

Copyright

© Mainz 2012, SI Analytics GmbH,
Nachdruck - auch auszugsweise - nur mit schriftlicher
Genehmigung der SI Analytics GmbH, Mainz.
Printed in Germany.

Ansicht Einstabmesskette SCHOTT® Instruments K 60



Inbetriebnahme

1	Schutzkappe entfernen.
2	Verschlussring nach unten ziehen, so dass die Nachfüllöffnung der Referenzelektrode frei ist.
3	Elektrolytlösung ELY/BR/503 in die Nachfüllöffnung einfüllen.
4	Schaft mit einem sauberen Papiertuch abwischen.
5	Messkette ca. 10 Minuten in entionisiertes Wasser stellen.
6	Messkette vor Gebrauch ca. 5 Minuten in verdünnte Standardlösung stellen. Eine Konzentration der Standardlösung knapp unterhalb des zu erwartenden Messbereichs ergibt eine kurze Ansprechzeit.

Die Messkette ist nun messbereit. Während der Messung die Nachfüllöffnung der Referenzelektrode immer offen lassen.

Kalibrieren

Nach den Angaben der Anleitung des Messgeräts und der Analysenvorschrift kalibrieren.

Probenvorbereitung

2 % ISA/K - Lösung zugeben. Diese Probenkonditionierlösung stellt die optimalen Bedingungen für die Messung ein. Sie sorgt für eine konstante Ionenstärke und gleiche Diffusionspotentiale an der Referenzelektrode in Standard und Messprobe.



Für detaillierte Angaben zu Probenvorbehandlung und

Messverfahren steht Ihnen bei SI Analytics eine große Anzahl an Applikationsberichten für die verschiedensten Anwendungen zur Verfügung.

Ansprechzeiten

Die Ansprechzeit hängt vom Konzentrationsbereich ab. Sie beträgt

- einige Sekunden bei hohen Konzentrationen,
- einige Minuten in der Nähe der Nachweisgrenze.

Der Messwert ist stabil, wenn sich der Wert innerhalb 30 Sekunden um nicht mehr als 0,1 mV ändert.

Störungen

Störungen: 10 % Fehler bei folgendem Konzentrationsverhältnis: (Konzentrationsverhältnis = Störion / Mession)

Cs ⁺	NH ₄ ⁺	Tl ⁺	H ⁺	Ag ⁺	Tris ⁺	Li ⁺	Na ⁺
0.3	6	6	10	1000	1000	2000	2000

Alterung

Beachten Sie bitte, dass jede Messkette bzw. Elektrode einer natürlichen Alterung unterliegt.

Mit dem Alter der Messkette bzw. Elektrode nimmt die Ansprechzeit zu und die Steilheit ab. Folgende Faktoren verkürzen die Lebensdauer erheblich:

- Unsachgemäße Lagerung
- Spezielle Messmedien (z. B. organische Lösungen, häufiges Messen bei hohen Störionenkonzentrationen)

- Hohe Temperaturen
- Große Temperaturwechsel

Für durch Messbedingungen verursachte Schäden und bei mechanischen Beschädigungen bestehen keine Garantieansprüche.


Wartung

- Bei Einstabmessketten verbrauchte Referenzelektrolytlösung ergänzen.
- Bei erhöhten Ansprechzeiten oder driftenden Messwerten die Messkette bzw. Elektrode eine Stunde in destilliertes Wasser stellen und anschließend mehrere Stunden in verdünnter Standardlösung aufbewahren.

Lagerung

- Zwischen zwei Messungen die Messkette in verdünnte Standardlösung stellen.
- Über Nacht bis zu einer Woche: Verschlussring nach oben schieben, um die Nachfüllöffnung zu verschließen. Anschließend die Messkette mit entionisiertem Wasser spülen, mit einem sauberen Papiertuch trocken tupfen und an einem trockenen Ort aufbewahren.
- Länger als eine Woche: Die Elektrolytflüssigkeit der Referenzelektrode entfernen und die Messkette mit entionisiertem Wasser spülen, mit einem sauberen Papiertuch trocken tupfen und die Schutzkappe aufsetzen. Die Messkette an einem trockenen Ort aufbewahren.

Typische Kalibrierkurve einer Kalium-Elektrode

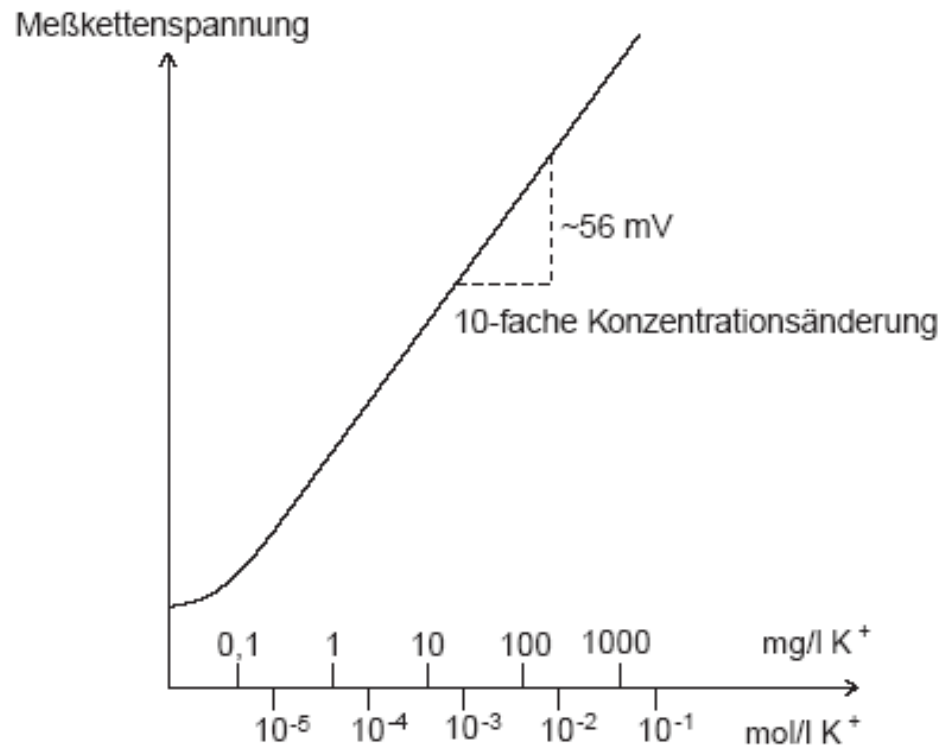

Technische Daten

SCHOTT® Instruments ISE - Einstabmesskette K 60

Messbereich 0,04 ... 39000 mg/l K⁺ (1 x 10⁻⁶ ... 1 mol/l K⁺)

Reproduzierbarkeit ± 2 %

pH-Bereich 2 ... 12 (siehe Abschnitt STÖRUNGEN)

Temperaturbereich 0 ... 40 °C

Membranwiderstand < 50 MΩ

Länge 170 mm (einschließlich 50 mm Anschlusskopf)

Durchmesser Schaft: 12 mm
Anschlusskopf 16 mm

Bedienungsanleitung / Operating Manual

**SCHOTT[®] Instruments
Combination Electrode**

K 60

Potassium Combination Electrode K 60

Accuracy when

going to press

The use of advanced technology and the high quality standard of our products are the result of a continuous development. This may result in differences between this operating manual and your electrode. Also, we cannot guarantee that there are absolutely no errors in this manual. Therefore, we are sure you will understand that we cannot accept any legal claims resulting from the data, figures or descriptions.

Warranty declaration

In case of proper handling, SI ANALYTICS guarantees the quality of the electrode for one year.

Copyright

© Mainz 2012, SI Analytics GmbH
Reprinting - even as excerpts - is only allowed with the explicit written authorization of SI Analytics GmbH, Mainz.
Printed in Germany.

View K 60 Potassium Combination Electrode



Commissioning

1	Remove the protection cap.
2	Pull the closing ring downwards so that the refilling opening of the reference electrode is free.
3	Fill ELY/BR/503 electrolyte solution into the refilling opening.
4	Wipe the shaft using a clean paper towel.
5	Place the combination electrode into deionized water for approx. 10 minutes.
6	Before use, place the combination electrode into diluted standard solution for approx. 5 minutes. In order to achieve a short response time, the concentration of the standard solution should be slightly below the measuring range expected.

The combination electrode is now ready to measure. Always leave the refilling opening of the reference electrode open while measuring.

Calibration

Calibrate according to the data given in the operating manual of the measuring instrument and the analysis specification.

Sample preparation

Add 2 % ISA/K solution. This sample conditioning solution creates optimum conditions for measuring. It provides a constant ionic strength and similar diffusion potentials at the reference electrode in standard and test sample.



If you would like to have more detailed information concerning sample preparation and measuring procedures, SI Analytics provides a large number of application reports for various applications.

Response times

The response time depends on the concentration range.

It is:

- several seconds with high concentrations,
- several minutes near the detection limit.

The measured value is stable if the value does not change by more than 0.1 mV within 30 seconds.

Interferences

Interfering ions: 10 % error with the following ratios of concentration: (Ratio of concentration = Interfering ion / Measuring ion)

Cs ⁺	NH ₄ ⁺	Tl ⁺	H ⁺	Ag ⁺	Tris ⁺	Li ⁺	Na ⁺
0.3	6	6	10	1000	1000	2000	2000

Aging

Please note that every electrode undergoes a natural aging process. The response time increases and the slope decreases with the age of the electrode. The following factors shorten the lifetime considerably:

- Incorrect storing
- Special measuring conditions (e.g. organic solutions, frequent measuring with high concentrations of interfering ions)
- High temperatures
- High changes in temperature

The warranty does not cover damage caused by measuring conditions and mechanical damage.

Maintenance


- For combination electrodes: replenish used reference electrolyte solution.
- In case of increased response times or drifting measured values, place the electrode into distilled water for one hour and then store it in diluted standard solution for several hours.

Storage

- Between two measurements, place the combination electrode into diluted standard solution.
- Overnight up to one week: Push the closing ring upwards to close the refilling opening. Then rinse the combination electrode with deionized water, blot it dry using a clean paper towel and store it in a dry place.

- For more than a week: Remove the electrolyte solution from the reference electrode and rinse the combination electrode with deionized water, blot it dry using a clean paper towel and put on the protection cap. Store the combination electrode in a dry place.

Typical calibration line of a potassium electrode

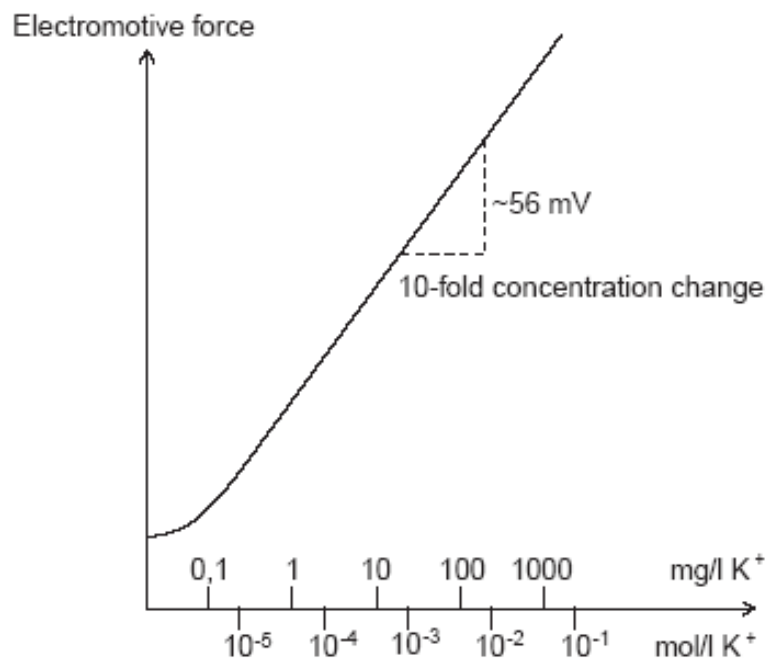

Technical data

SCHOTT[®] Instruments ISE - Combination Electrode **CI 60**

Measuring range 0.04 ... 39000 mg/l K⁺ (1 x 10⁻⁶ ... 1 mol/l K⁺)

Reproducibility ± 2 %

pH range 2 ... 12 (see section INTERFERENCES)

Temperature range 0 ... 40 °C

Membrane resistance < 50 MΩ

Length 170 mm (including 50 mm connection head)

Diameter Shaft: 12 mm
Connection head: 16 mm

Notizen / Notes

SI Analytics

a **xylem** brand

SI Analytics GmbH

Hattenbergstrasse 10

55122 Mainz

Germany

Phone: +49 (0) 6131/66 5111

Telefax: +49 (0) 6131/66 5001

E-mail: support.si-analytics@xylem.com

Internet: www.si-analytics.com

T814844